

RESMED

 **DirectHome
MEDICAL**

Presented With Compliments From
www.DirectHomeMedical.com



Have you heard?

Mirage Swift™ II is better than ever.

**So light, so flexible, so quiet ...
Mirage Swift II is better than ever!**


The Mirage Swift II nasal pillows system is now 86% quieter than the Mirage Swift.* It is designed to direct air away from the patient and the bed partner for quiet and gentle therapy.

Not only is the Mirage Swift II quieter, but the vent direction is angled downward in a direction more aligned with the flow of natural breath.




To illustrate how an 86% decrease in noise level may be perceived by the ear, the noise level may be equated to:

Swift:
A person
whispering
3 feet (1 m)
away from you

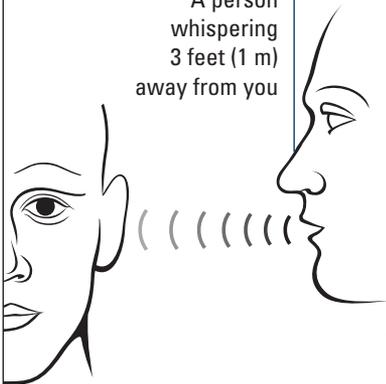

Swift II:
A person
whispering
10 feet (3 m)
away from you

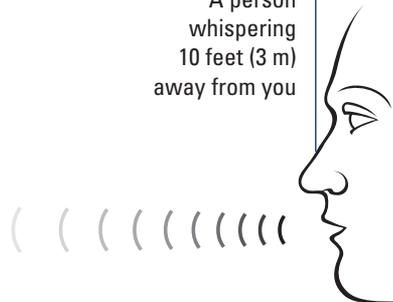

Conclusion: The Mirage Swift II is significantly quieter than the Mirage Swift.

* Source: Testing Per ISO 3744:1994 Acoustics Determination of Sound power levels of noise sources using sound pressure.

Mirage Swift II ... what's new and different ?

This simple guide identifies the product differences between Mirage Swift and Swift II.

Pillows

Is the ResMed logo molded on the front, or are there six vent holes?

Frame



Does the frame have two rows of small vent holes, or is it solid?

Frame clip

Does the clip have an opening in it, or is it solid?

End cap

Is the end cap blue or clear?

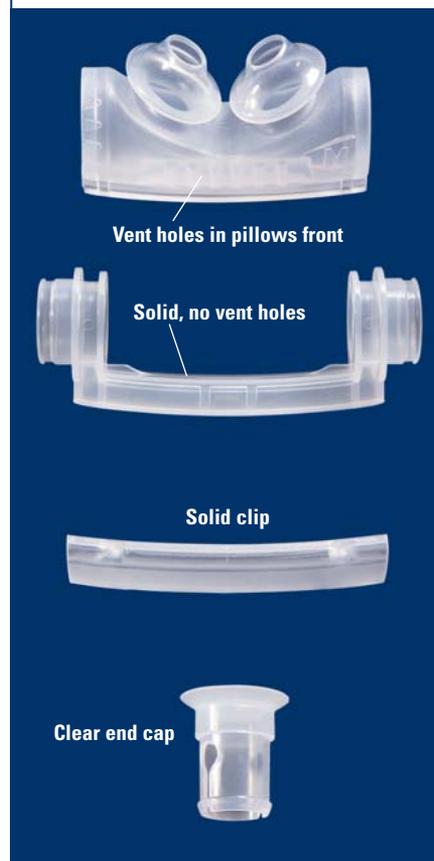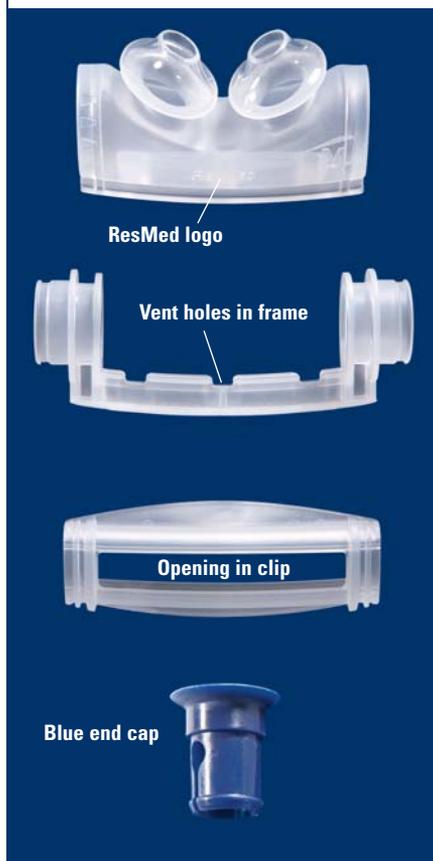

If you would like to purchase a complete system of the Mirage Swift II, the new product code for US, Canada and Latin America is **60512**.

For questions regarding the Mirage Swift or Mirage Swift II, or to place an order, please contact your local ResMed sales representative or call Customer Service at 800.424.0737.