

# Making it simple to find the right fit

Achieving the right fit with DreamWear is easy



## Nasal cushion sizing

Using the nasal cushion sizing gauge (included with the mask), hold it horizontally under the nose. Select the cushion size based on where the outer edge of the nostrils and tip of the nose contact the gauge.

Note: Four cushion sizes (small, medium, large, medium-wide) are available.


## Gel pillows cushion sizing

Using the gel pillows sizing gauge, place the pillows cushion tips into the nostrils. Choose the cushion size that allows the blue gel bases to sit comfortably under the nose without any gaps.


Note: Three cushion sizes (small, medium, large) are available.

### Medium frame sizing


The medium mask frame will comfortably fit most faces. If the medium frame does not fit a patient's face, a small or large mask frame might better suit your patient's needs.

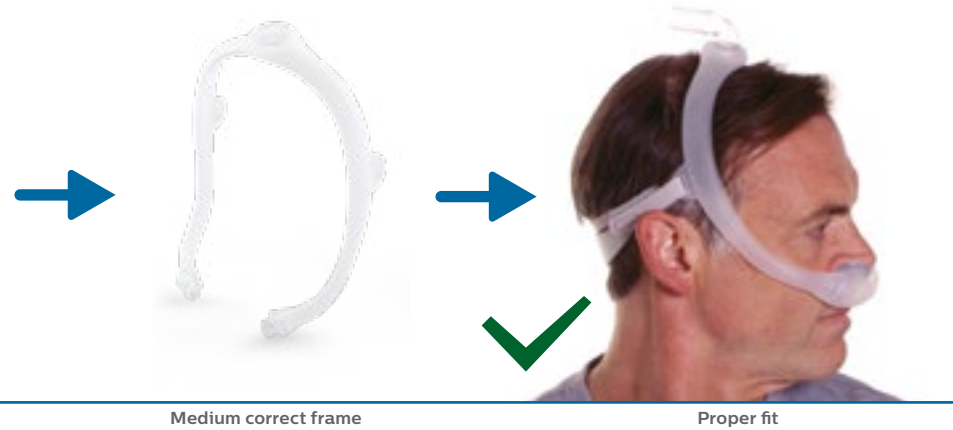

### Large frame sizing

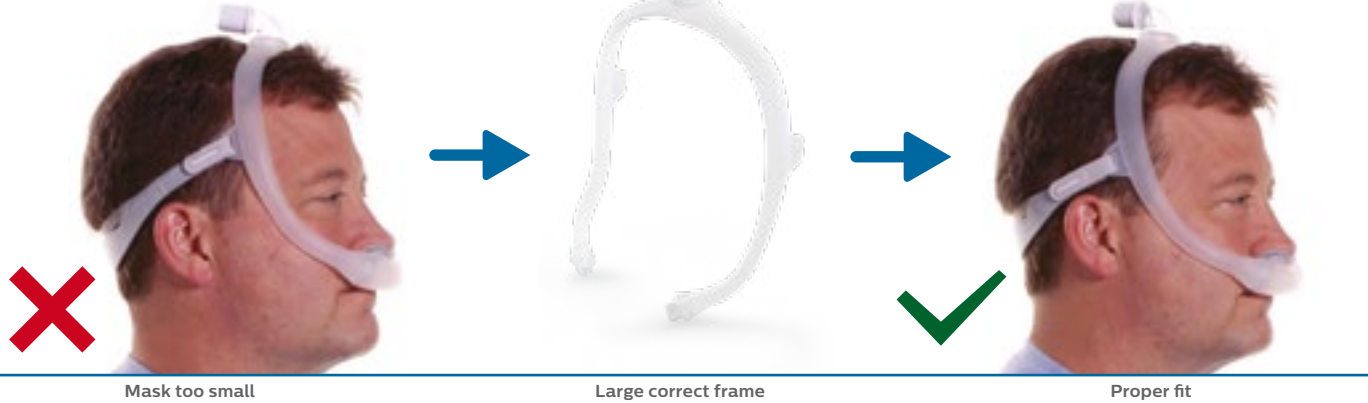

### Small frame sizing

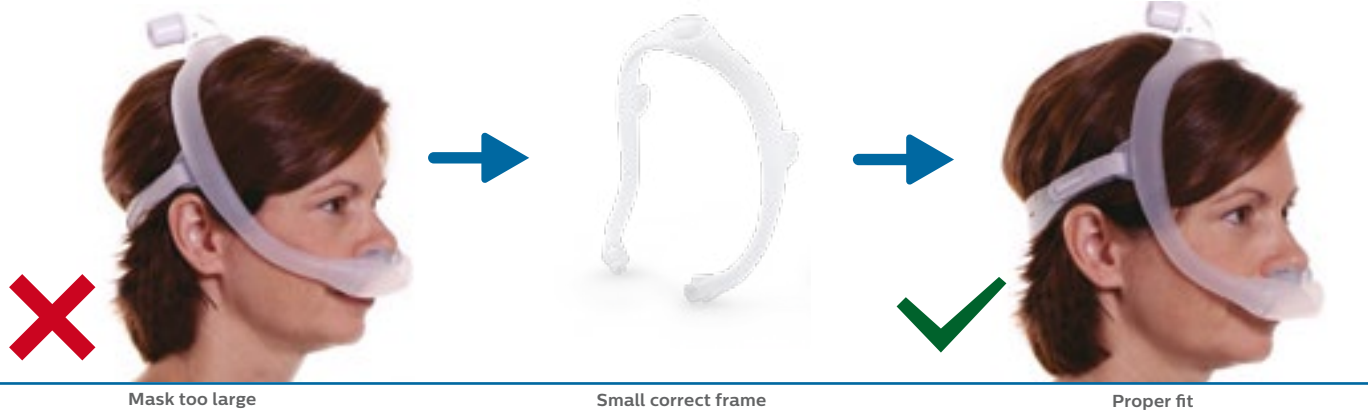

# DreamWear cushion patient fitting guide


Follow the instructions to get started fitting your nasal or gel pillows cushion

## Nasal cushion



The cushion opening will be directly under the nostrils. The cushion will hug the nose and leak will be minimal.

Note: At no time should the nose be inside the cushion opening. If any part of the cushion overlaps the nose, the cushion is being worn incorrectly.

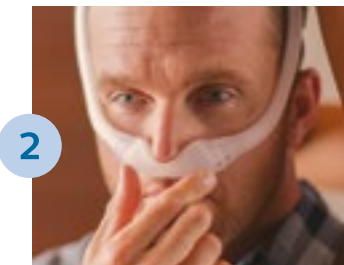

With the mask assembled, place the cushion under the nose.




Position the frame on the top of the head. Pull the headgear over the back of the head.




To adjust the mask, peel the headgear tabs away from the fabric. Adjust the length of the straps. Press the tabs back against the fabric to reattach.

Note: Do not overtighten the headgear.

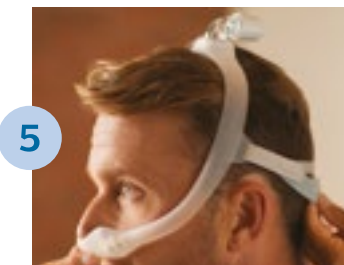

Position the mask until it fits comfortably.

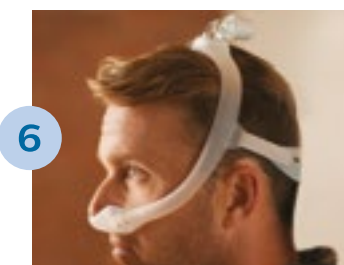

When finished, the elbow should rest at the top of the head.

Note: Please read the Instructions for Use for further fitting information.

## Gel pillows cushion

